

PHYSICS



EXAM QUESTION PACK

24 MEDICAL PHYSICS

SCORE

/

PERCENTAGE

%

STEMUP

These questions belong to CIE, not to us.

The examination questions, mark schemes and examiner comments in this pack were written and published by Cambridge International (CIE). They are past assessment materials, reproduced here so that students can revise from them.

What we do not own

STEMUP is not affiliated with CIE and does not own, and makes no claim to own, any of the question, mark scheme or examiner report material in this pack. CIE has not endorsed, approved or been involved in the production of it. CIE and the qualification titles used here belong to their respective owners and appear for identification only.

Where to find the originals

CIE publishes its past papers, mark schemes and examiner reports. Always check the current syllabus at [cambridgeinternational.org](https://www.cambridgeinternational.org) before you revise.

If you hold the rights to any material in this pack and would like it amended or removed, contact admin@stemup.co.uk and we will act on it.

Q1.

- 7 (a) Briefly explain the principles of the production of an X-ray beam.

.....
.....
.....
.....
.....
.....
..... [5]

- (b) State how, in an X-ray tube,

- (i) the intensity of the X-ray beam may be increased,

.....

- (ii) the X-ray beam may be made more penetrating,

.....

- (iii) the unwanted 'soft' X-rays may be removed from the beam.

..... [3]

- (c) The intensity of a parallel X-ray beam is reduced to one half of its initial intensity when it passes through bone of thickness 0.40 cm. Calculate the thickness of bone necessary to reduce the beam intensity to one tenth of its initial value.

thickness = ... cm [3]

Q2.

8 Suggest why, when using a laser as a scalpel,

(a) the laser beam is focused using a short focal length convex lens,

.....
.....
..... [2]

(b) less bleeding is caused than when using a knife.

.....
.....
..... [2]

Q3.

9 (a) Explain what is meant by the *sensitivity* of the ear.

.....
.....
..... [2]

(b) A person stands in a room where the intensity of the background noise due to a party is $4.5 \times 10^{-5} \text{ W m}^{-2}$. The smallest change in intensity level of sound that can be detected by the person is 3.0 dB.

Calculate the change in intensity of sound necessary for the person to hear someone else speak above the background noise.

change = ... W m^{-2} [3]

Q4.

- 9 (a) Explain the principles behind the use of X-rays for imaging internal body structures.

.....

.....

.....

.....

.....

.....

..... [4]

- (b) Describe how the image produced during CT scanning differs from that produced by X-ray imaging.

.....

.....

.....

.....

.....

.....

..... [5]

Q5.

10 Outline briefly the main principles of the use of magnetic resonance to obtain information about internal body structures.

For
Examin
Use

[8]

Q6.

- 11 (a) Explain the main principles behind the **use** of ultrasound to obtain diagnostic information about internal body structures.

For
Examiner's
Use

.....

.....

.....

.....

.....

.....

.....

.....

.....

..... [4]

- (b) Data for the acoustic impedances and absorption (attenuation) coefficients of muscle and bone are given in Fig. 11.1.

	acoustic impedance / $\text{kg m}^{-2} \text{s}^{-1}$	absorption coefficient / m^{-1}
muscle	1.7×10^6	23
bone	6.3×10^6	130

Fig. 11.1

The intensity reflection coefficient is given by the expression

$$\frac{(Z_2 - Z_1)^2}{(Z_2 + Z_1)^2}.$$

The attenuation of ultrasound in muscle follows a similar relation to the attenuation of X-rays in matter.

A parallel beam of ultrasound of intensity I enters the surface of a layer of muscle of thickness 4.1 cm as shown in Fig. 11.2.

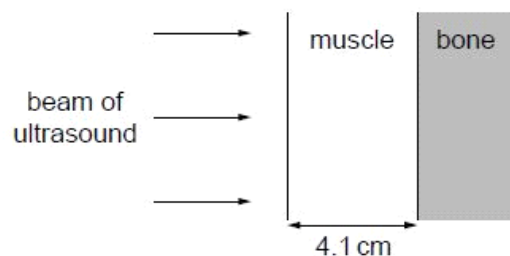


Fig. 11.2

The ultrasound is reflected at a muscle-bone boundary and returns to the surface of the muscle.

Calculate

- (i) the intensity reflection coefficient at the muscle-bone boundary,

coefficient = ... [2]

- (ii) the fraction of the incident intensity that is transmitted from the surface of the muscle to the surface of the bone,

fraction = ... [2]

- (iii) the intensity, in terms of I , that is received back at the surface of the muscle.

intensity = ... I [2]

Q7.

10 (a) Briefly explain the principles of CT scanning.

Ex

..[6]

(b) A simple section through a body consists of four voxels, as illustrated in Fig. 10.1.

Exam Us

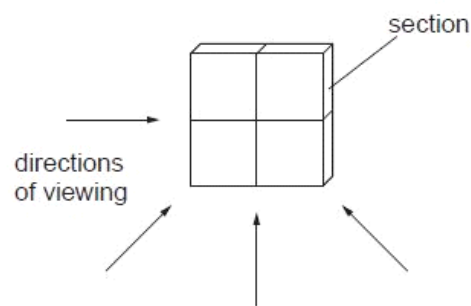


Fig. 10.1

An X-ray image of the section is obtained by viewing along each of the directions shown in Fig. 10.1.

The detector readings for each direction of viewing are summed to give the pattern of readings shown in Fig. 10.2.

25	22
34	31

Fig. 10.2

(i) For the pattern of readings of Fig. 10.2, state the magnitude of the background reading.

(ii) On Fig. 10.1, mark the pattern of pixels for the four-voxel section. [2]

11 Explain the main principles behind the **generation** of ultrasound to obtain diagnostic information about internal body structures.

..... [6]

STEMUP.CO.UK

- 10 (a) State what is meant by the *acoustic impedance* Z of a medium.

.....
.....[1]

- (b) Two media have acoustic impedances Z_1 and Z_2 .
The intensity reflection coefficient α for the boundary between the two media is given by

$$\alpha = \frac{(Z_2 - Z_1)^2}{(Z_2 + Z_1)^2}.$$

Describe the effect on the transmission of ultrasound through a boundary where there is a large difference between the acoustic impedances of the two media.

.....
.....
.....
.....[3]

- (c) Data for the acoustic impedance Z and the absorption coefficient μ for fat and for muscle are shown in Fig. 10.1.

	$Z/\text{kg m}^{-2}\text{s}^{-1}$	μ/m^{-1}
fat	1.3×10^6	48
muscle	1.7×10^6	23

Fig. 10.1

The thickness x of the layer of fat on an animal, as illustrated in Fig. 10.2, is to be investigated using ultrasound.

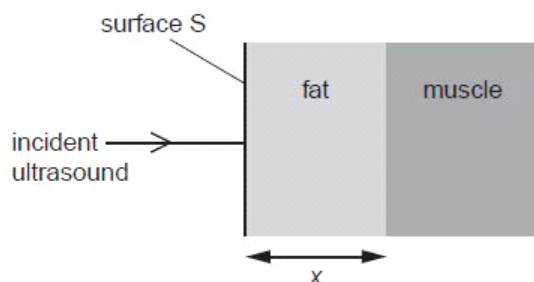


Fig. 10.2

The intensity of the parallel ultrasound beam entering the surface S of the layer of fat is I .
The beam is reflected from the boundary between fat and muscle.
The intensity of the reflected ultrasound detected at the surface S of the fat is $0.012 I$.
Calculate

For
Examin
Use

- (i) the intensity reflection coefficient at the boundary between the fat and the muscle,

coefficient = ... [2]

- (ii) the thickness x of the layer of fat.

x = ... cm [3]

Q10.

- 10 Explain briefly the main principles of the use of magnetic resonance to obtain diagnostic information about internal body structures.

For
Examin
Use

[8]

Q11.

- 11 High-speed electrons are incident on a metal target. The spectrum of the emitted X-ray radiation is shown in Fig. 11.1.

Exam Us

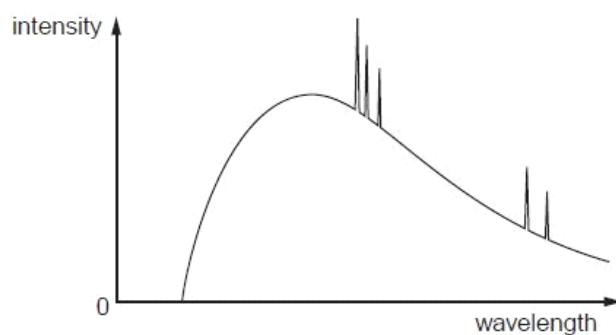


Fig. 11.1

- (a) Explain why
- (i) there is a continuous distribution of wavelengths,

[2]

(ii) there is a sharp cut-off at short wavelength.

.....
.....
..... [2]

(b) State

(i) what is meant by the *hardness* of an X-ray beam,

.....
.....
..... [2]

(ii) how hardness is controlled.

.....
.....
..... [2]

(c) (i) Suggest why, when producing an X-ray image, long-wavelength X-ray radiation poses a greater hazard to health than short-wavelength radiation.

Ex

.....
..... [1]

(ii) Suggest how this hazard is minimised.

.....
..... [1]

Q12.

12 A person is to be investigated using a magnetic resonance (MR) scanner.

For
Examine
Use

- (a) This technique involves the use of two superimposed magnetic fields.
Describe the functions of these two magnetic fields.

.....

.....

.....

.....

.....

..... [4]

- (b) The frequency f of the electromagnetic waves emitted by protons on relaxation in an MR scanner is given by the equation

$$f = 2cB$$

where B is the total magnetic flux density and c is a constant equal to $1.34 \times 10^8 \text{ s}^{-1} \text{ T}^{-1}$.
The magnetic flux density changes by $2.0 \times 10^{-4} \text{ T}$ for each 1.0 cm thickness of tissue in a section.

The scanner is adjusted so that the thickness of each section is 3.0 mm.

Calculate, for corresponding points in neighbouring sections,

Calculate, for corresponding points in neighbouring sections,

- (i) the difference in magnetic flux density,

difference in flux density = ... T [1]

- (ii) the change in emitted frequency.

frequency change = ... Hz [2]

Q13.

- 10 (a) An aluminium block is placed near to a small source of X-ray radiation, as shown in Fig. 10.1.

Ex

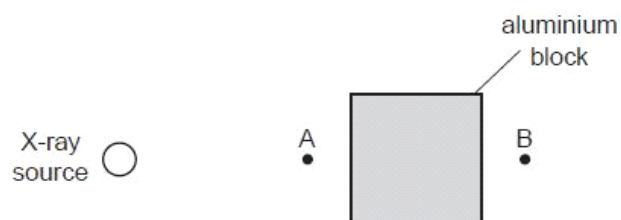


Fig. 10.1

X-rays from the source are detected at point A and at point B.

State two reasons why the intensity of the X-ray beam at point B is not as great as the intensity at point A.

1.
2.

[2]

- (b) A cross-section through a model of a finger is shown in Fig. 10.2.

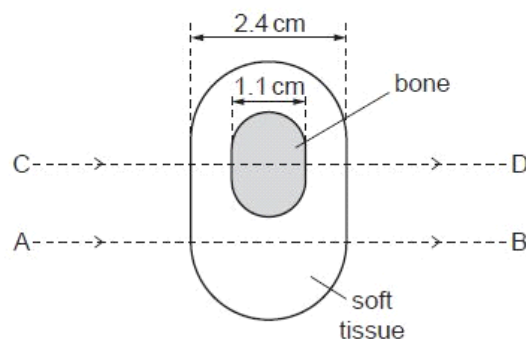


Fig. 10.2

The thickness of the model is 2.4 cm and that of the bone in the model is 1.1 cm. Parallel beams of X-rays are incident on the model in the directions AB and CD, as shown in Fig. 10.2.

Data for the linear attenuation (absorption) coefficient μ for the bone and the soft tissue in the model are given in Fig. 10.3.

For
Examin
Use

	μ / cm^{-1}
bone	3.0
soft tissue	0.27

Fig. 10.3

Calculate the ratio

$$\frac{\text{intensity of X-ray beam incident on the model}}{\text{intensity of X-ray beam emergent from the model}}$$

for

(i) the beam AB,

ratio = ...[2]

(ii) the beam CD.

ratio = ...[2]

- (c) Use your answers in (b) to suggest why, for this model, an X-ray image with good contrast may be obtained.

.....
[1]

Q14.

- 10 (a) Distinguish between sharpness and contrast in X-ray imaging.

sharpness:

 contrast:
[2]

For
Examiner
Use

- (b) State two causes of loss of sharpness of an X-ray image.

1.

 2.
[2]

- (c) Data for the linear attenuation (absorption) coefficient μ of X-ray photons are given in Fig. 10.1.

	μ/cm^{-1}
bone	2.85
muscle	0.95

Fig. 10.1

A parallel beam of X-rays is incident, separately, on a thickness of 3.5 cm of bone and on a muscle of thickness 8.0 cm.

- (i) Calculate the ratio

$$\frac{\text{intensity of X-ray beam transmitted through bone}}{\text{intensity of X-ray beam transmitted through muscle}}$$

ratio = ... [3]

- (ii) Use your answer in (i) to suggest whether an X-ray image of the bone and muscle would show good or poor contrast.

.....

 [2]

*Ft
Exam
Ut*

Q15.

- 10 (a) By reference to ultrasound waves, state what is meant by *acoustic impedance*.

For
Examine
Use

.....
.....
..... [2]

- (b) An ultrasound wave is incident on the boundary between two media. The acoustic impedances of the two media are Z_1 and Z_2 , as illustrated in Fig. 10.1.

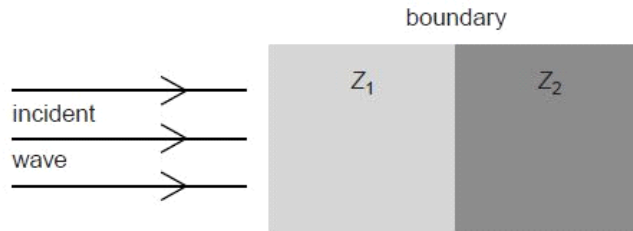


Fig. 10.1

Explain the importance of the difference between Z_1 and Z_2 for the transmission of ultrasound across the boundary.

.....
.....
..... [3]

- (c) Ultrasound frequencies as high as 10MHz are used in medical diagnosis. State and explain one advantage of the use of high-frequency ultrasound compared with lower-frequency ultrasound.

.....
.....
..... [2]

Q16.

- 11 (a) Explain how the hardness of an X-ray beam is controlled by the accelerating voltage in the X-ray tube.

For
Examiner's
Use

.....
.....
..... [2]

- (b) The attenuation of a parallel beam of X-ray radiation is given by the expression

$$\frac{I}{I_0} = e^{-\mu x}$$

where μ is the linear attenuation (absorption) coefficient and x is the thickness of the material through which the beam passes.

- (i) State

1. what is meant by *attenuation*,

.....
..... [1]

2. why the expression applies only to a parallel beam.

.....
.....
..... [2]

- (ii) The linear attenuation coefficients for X-rays in bone and in soft tissue are 2.9 cm^{-1} and 0.95 cm^{-1} respectively.

Calculate, for a parallel X-ray beam, the ratio

$$\frac{\text{fraction } \frac{I}{I_0} \text{ of intensity transmitted through bone of thickness } 2.5 \text{ cm}}{\text{fraction } \frac{I}{I_0} \text{ of intensity transmitted through soft tissue of thickness } 6.0 \text{ cm}}.$$

ratio = ... [2]

Q17.

9 (a) State what is meant by *acoustic impedance*.

.....
.....[1]

(b) Explain why acoustic impedance is important when considering reflection of ultrasound at the boundary between two media.

.....
.....
.....[2]

(c) Explain the principles behind the use of ultrasound to obtain diagnostic information about structures within the body.

.....
.....
.....
.....
.....
.....
.....
.....[5]

Q18.

11 (a) Distinguish between the images produced by CT scanning and X-ray imaging.

For
Examinee
Use

.....

.....

.....

..... [3]

(b) By reference to the principles of CT scanning, suggest why CT scanning could not be developed before powerful computers were available.

.....

.....

.....

.....

.....

.....

.....

..... [5]

Q19.

11 Outline briefly the main principles of the use of magnetic resonance to obtain diagnostic information about internal body structures.

For
Examiner's
Use

.....

.....

.....

.....

.....

.....

.....

.....

.....

.....

.....

..... [6]

Q20.

- 10 (a) A typical spectrum of the X-ray radiation produced by electron bombardment of a metal target is illustrated in Fig. 10.1.

For
Examiner
Use

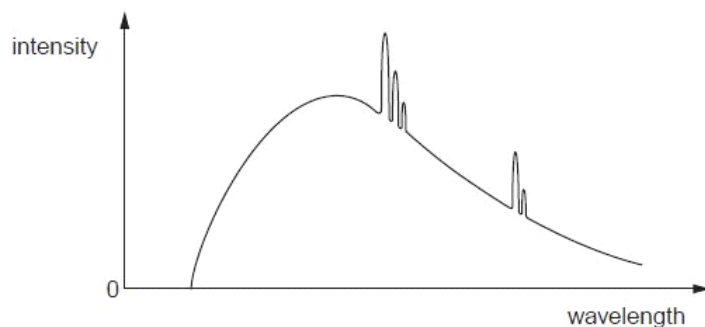


Fig. 10.1

Explain why

- (i) a continuous spectrum of wavelengths is produced,

.....
.....
.....
..... [3]

- (ii) the spectrum has a sharp cut-off at short wavelengths.

.....
..... [1]

- (b) The variation with photon energy E of the linear absorption coefficient μ of X-rays in soft tissue is illustrated in Fig. 10.2.

For
Examiner:
Use

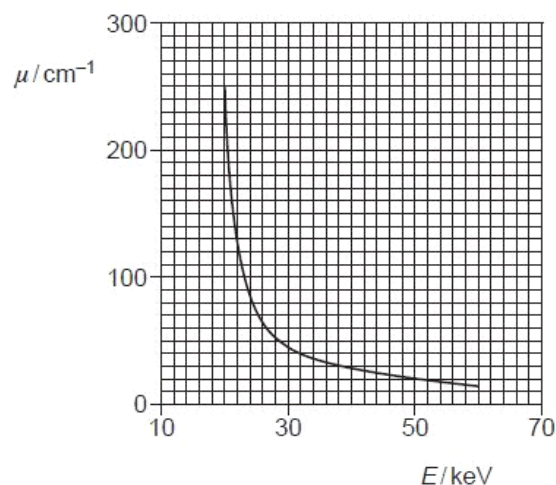


Fig. 10.2

- (i) Explain what is meant by *linear absorption coefficient*

.....

 [3]

- (ii) For one particular application of X-ray imaging, electrons in the X-ray tube are accelerated through a potential difference of 50 kV.

Use Fig. 10.2 to explain why it is advantageous to filter out low-energy photons from the X-ray beam.

.....

 [3]

Q21.

- 10 (a) (i) State what is meant by the *acoustic impedance* of a medium.

For
Examiner
Use

.....
.....[1]

- (ii) Data for some media are given in Fig. 10.1.

medium	speed of ultrasound / ms^{-1}	acoustic impedance / $\text{kg m}^{-2} \text{s}^{-1}$
air	330	4.3×10^2
gel	1500	1.5×10^6
soft tissue	1600	1.6×10^6
bone	4100	7.0×10^6

Fig. 10.1

Use data from Fig. 10.1 to calculate a value for the density of bone.

density = ... kg m^{-3} [1]

- (b) A parallel beam of ultrasound has intensity I . It is incident at right-angles to a boundary between two media, as shown in Fig. 10.2.

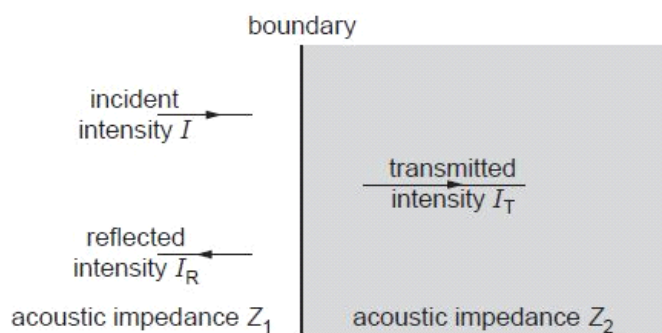


Fig. 10.2

The media have acoustic impedances of Z_1 and Z_2 . The transmitted intensity of the ultrasound beam is I_T and the reflected intensity is I_R .

- (i) State the relation between I , I_T and I_R .

.....[1]

- (ii) The reflection coefficient α is given by the expression

$$\alpha = \frac{(Z_2 - Z_1)^2}{(Z_2 + Z_1)^2}.$$

Use data from Fig. 10.1 to determine the reflection coefficient α for a boundary between

1. gel and soft tissue,

$\alpha =$ [2]

2. air and soft tissue.

$\alpha =$ [1]

- (c) By reference to your answers in (b)(ii), explain the use of a gel on the surface of skin during ultrasound diagnosis.

.....
.....
.....
.....[3]

Q22.

9 (a) (i) State, with reference to X-ray images, what is meant by *sharpness*.

.....
.....[1]

(ii) Describe briefly two factors that affect the sharpness of an X-ray image.

1.
.....
2.
.....
[3]

(b) An X-ray image is taken of the skull of a patient. Another patient has a CT scan of his head.

By reference to the formation of the image in each case, suggest why the exposure to radiation differs between the two imaging techniques.

.....
.....
.....
.....
.....[4]

Q23.

- 11 The linear attenuation (absorption) coefficient μ for X-ray radiation in bone, fat and muscle is given in Fig. 11.1.

For
Examiner's
Use

	μ / cm^{-1}
bone	2.9
fat	0.90
muscle	0.95

Fig. 11.1

- (a) A parallel X-ray beam of intensity I_0 is incident either on some bone or on some muscle.

The emergent beam has intensity I .

Calculate the ratio $\frac{I}{I_0}$ for a thickness of

- (i) 1.5 cm of bone,

ratio = ... [2]

- (ii) 4.6 cm of muscle.

ratio = ... [1]

- (b) Suggest why, on an X-ray plate, the contrast between bone and muscle is much greater than that between fat and muscle.

.....

 [3]

Q24.

10 Explain the principles of the generation and detection of ultrasound waves.

For
Exami
Us

[6]

Q25.

11 (a) Distinguish between *sharpness* and *contrast* in X-ray imaging.

For
Examiner's
Use

sharpness:

contrast:

[2]

(b) A student investigates the absorption of X-ray radiation in a model arm. A cross-section of the model arm is shown in Fig. 11.1.

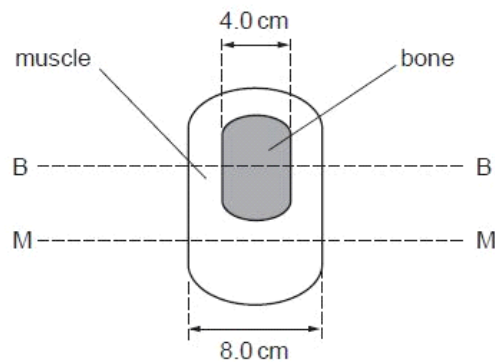


Fig. 11.1

Parallel X-ray beams are directed along the line MM and along the line BB.
The linear absorption coefficients of the muscle and of the bone are 0.20 cm^{-1} and 12 cm^{-1} respectively.

Calculate the ratio

$$\frac{\text{intensity of emergent X-ray beam from model}}{\text{intensity of incident X-ray beam on model}}$$

for a parallel X-ray beam directed along the line

(i) MM,

ratio = ... [2]

(ii) BB.

For
Examiner's
Use

ratio = ... [3]

(c) State whether your answers in (b) would indicate that the X-ray image

(i) is sharp,

..... [1]

(ii) has good contrast.

..... [1]

Q26.

10 Outline the principles of CT scanning.

For
Examiner's
Use

..... [6]

Q27.

10 A simple model of one section of a CT scan is shown in Fig. 10.1.

For
Examine
Use

A	B
D	C

Fig. 10.1

The model consists of four voxels with pixel numbers A , B , C and D .

In this model, the voxels are viewed in turn along four different directions D_1 , D_2 , D_3 and D_4 as shown in Fig. 10.2.

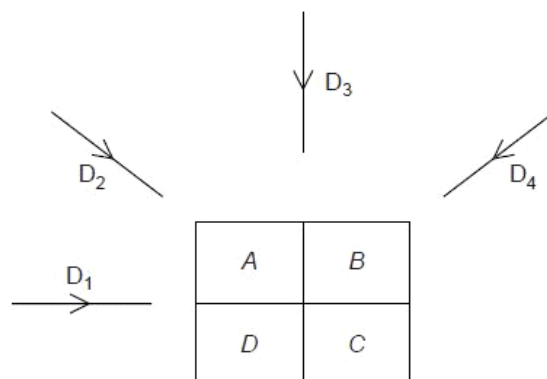


Fig. 10.2

The pixel readings in each of the four directions are noted.
 The total pixel reading for any one direction is 19.
 The pixel readings for all of the directions are summed to give the pattern of readings shown in Fig. 10.3.

25	34
28	46

Fig. 10.3

(a) State the background reading in this model.

background reading = ...[1]

(b) Determine each of the pixel readings.

A = ...	B = ...
D = ...	C = ...

[4]

(c) Use your answers in (b) to determine the pixel readings along

(i) the direction D₃,
[1]

(ii) the direction D₄.
[2]

For
Examiner:
Use

Q28.

10 (a) Explain the main principles behind the **use** of ultrasound to obtain diagnostic information about internal body structures.

(b) State and explain one advantage of the use of high frequency ultrasound as compared with low frequency ultrasound for medical diagnosis.

(c) The absorption (attenuation) coefficient for ultrasound in muscle is 23 m^{-1} . A parallel beam of ultrasound is passed through a muscle of thickness 6.4 cm .

$$\frac{\text{intensity of transmitted beam}}{\text{intensity of incident beam}}$$

STEMUP.CO.UK

- (ii) An ultrasound transmitter emits a pulse.
Suggest why, when the signal from the pulse is processed, any signal received later at the detector is usually amplified more than that received at an earlier time.

For
Examiner's
Use

.....

.....

.....[2]

Q29.

- 10 Magnetic resonance imaging (MRI) requires the use of a non-uniform magnetic field superimposed on a large uniform magnetic field.

For
Examiner's
Use

State and explain the purpose of

- (a) the large uniform magnetic field,

.....

.....

.....

.....

.....[3]

- (b) the non-uniform magnetic field.

.....

.....

.....

.....

.....[3]

Q30.

12 (a) Outline briefly the principles of CT scanning.

.....

.....

.....

.....

.....

.....

.....

.....

.....

.....

..... [5]

(b) In a model for CT scanning, a section is divided into four voxels. The pixel numbers P , Q , R and S of the voxels are shown in Fig. 12.1.

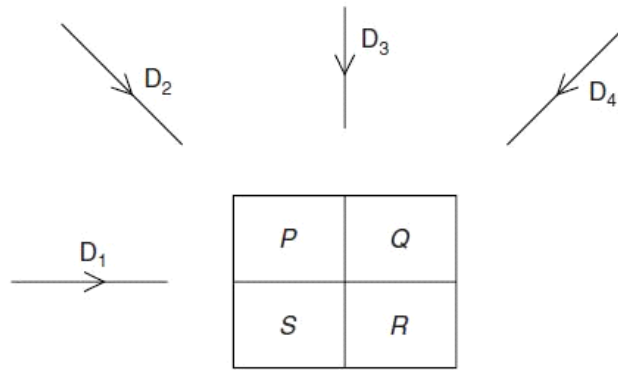


Fig. 12.1

The section is viewed from the four directions D_1 , D_2 , D_3 and D_4 . The detector readings for each direction are noted.

The detector readings are summed as shown in Fig. 12.2.

49	61
73	55

Fig. 12.2

The background reading is 34.

Determine the pixel numbers P , Q , R and S as shown in Fig. 12.3.

P	Q
S	R

Fig. 12.3

$P =$ $Q =$
 $S =$ $R =$

[4]

Q31.

- 11 (a) Distinguish between an X-ray image of a body structure and a CT scan.

X-ray image:

 CT scan:

[5]

- (b) Data for the linear absorption (attenuation) coefficient μ of X-ray radiation of energy 80keV are given in Fig. 11.1.

metal	μ / mm^{-1}
aluminium	0.46
copper	0.69

Fig. 11.1

A parallel X-ray beam is incident on a copper filter, as shown in Fig. 11.2.

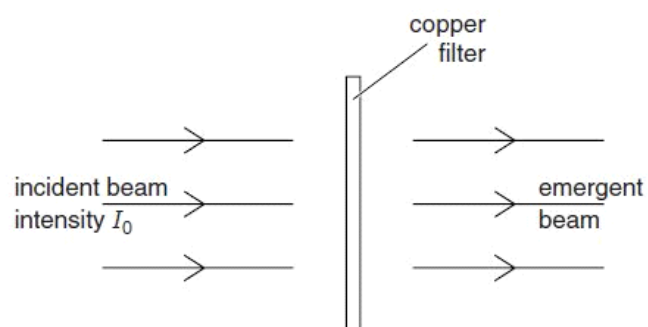


Fig. 11.2

The intensity of the incident beam is I_0 .

-
- (i) Calculate the thickness of copper required to reduce the intensity of the emergent beam to $0.25 I_0$.

thickness = ... mm [2]

- (ii) An aluminium filter of thickness 2.4 mm is now placed in the X-ray beam, together with the copper filter in (i).

Calculate the fraction of the incident intensity that emerges after passing through the two filters.

fraction = ... [2]

- (iii) Express your answer in (ii) as a gain in decibels (dB).

gain = ... dB [3]

Q32.

-
- 11 The use of X-rays in medical diagnosis gives rise to an increased exposure of the patient to radiation.

Explain why

- (a) an aluminium filter may be placed in the X-ray beam when producing an X-ray image of a patient,

.....
.....
.....
.....
..... [3]

- (b) the radiation dose received by a patient is different for a CT scan from that for a simple X-ray image.

.....
.....
.....
.....
.....
..... [4]

Q33.

- 11 (a) By reference to ultrasound waves, state what is meant by the *specific acoustic impedance* of a medium.

.....

 [2]

- (b) A parallel beam of ultrasound of intensity I is incident normally on a muscle of thickness 3.4 cm, as shown in Fig. 11.1.

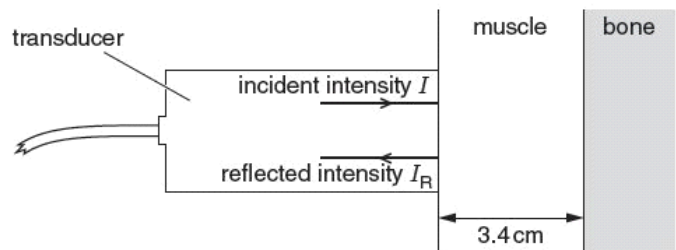


Fig. 11.1

The ultrasound wave is reflected at a muscle-bone boundary. The intensity of the ultrasound received back at the transducer is I_R .

Some data for bone and muscle are given in Fig. 11.2.

	specific acoustic impedance / $\text{kg m}^{-2} \text{s}^{-1}$	linear absorption coefficient / m^{-1}
bone	6.4×10^6	130
muscle	1.7×10^6	23

Fig. 11.2

- (i) The intensity reflection coefficient α for two media having specific acoustic impedances Z_1 and Z_2 is given by

$$\alpha = \frac{(Z_1 - Z_2)^2}{(Z_1 + Z_2)^2}.$$

Calculate the fraction of the ultrasound intensity that is reflected at the muscle-bone boundary.

fraction = ... [2]

-
- (ii) Calculate the fraction of the ultrasound intensity that is transmitted through a thickness of 3.4 cm of muscle.

fraction = ... [3]

- (iii) Use your answers in (i) and (ii) to determine the ratio $\frac{I_R}{I}$.

ratio = ... [2]

Q1.

- 7 (a) electrons fired at metal target B1
 electrons decelerated giving off (e.m.) radiation..... B1
 range of decelerations, so continuous spectrum..... B1
 also, electrons in inner orbits are excited..... B1
 de-excitation gives characteristic line spectrum B1 [5]
- (b) (i) increase cathode/tube current..... B1
 (ii) increase anode voltage..... B1
 (iii) use aluminium filter (allow metal filter) B1 [3]
- (c) $I = I_0 e^{-\mu x}$ C1
 $\ln 2 = 0.40\mu$
 $\mu = 1.733 \text{ cm}^{-1}$ or $= \ln 2 / 0.4$ C1
 $0.1 = e^{-1.733x}$
 $x = 1.33 \text{ cm}$ A1 [3]

Q2.

- 8 (a) produces greater intensity (at focus)
 limits region of cell damage
 allows for accurate guidance B2 [2]
- (b) laser beam cauterises tissue
 can produce coagulation
 vaporisation of water in cells..... B2 [2]
 {in (a) and (b), allow 1 mark each up to max of 3 in either, total not to exceed 4}

Q3.

- 9 (a) ability to detect (small) changes in loudness/intensity..... B1
 depends on $I / \Delta I$ B1 [2]
- (b) $\Delta I / I = 10 \lg(\Delta I / I)$ or $I / I_0 = 10 \lg(I / I_0)$ C1
 $3.0 = 10 \lg(I_2 / (4.5 \times 10^{-5}))$ C1
 $I_2 = 9.0 \times 10^{-5} \text{ W m}^{-2}$, $\Delta I = 4.5 \times 10^{-5} \text{ W m}^{-2}$ A1 [3]

Q4.

- 9 (a) X-ray beam directed through body onto detector (plate) B1
different tissues absorb/attenuate beam by different amounts B1
giving 'shadow' image of structures B1
any other detail e.g. comment re sharpness or contrast B1 [4]
- (b) X-ray image is flat OR 2-dimensional (1)
CT scan takes many images of a slice at different angles (1)
these build up an image of a slice through the body (1)
series of images of slices is made (1)
so that 3D image can be built up (1)
image can then be rotated (1)
1 mark for each point, max 5 B5 [5]

Q5.

- 10 large / strong (constant) magnetic field B1
nuclei rotate about direction of field / precess (1)
radio frequency / r.f. pulse B1
causes resonance in nuclei , nuclei absorb energy (1)
(pulse) is at the Larmor frequency (1)
on relaxation / nuclei de-excite emit (pulse of) r.f. B1
detected and processed B1
non-uniform field (superimposed) B1
allows for position of nuclei to be determined B1
and for location of detection to be changed (1)
(B6 plus any two extra details, 1 each, max 2) B2 [8]

Q6.

- 11 (a) pulse of ultrasound (1)
reflected at boundaries / boundary (1)
received / detected (at surface) by transducer (1)
signal processed and displayed (1)
time between transmission and receipt of pulse gives
(information about) depth of boundary (1)
reflected intensity gives information as to nature of boundary (1)
(any four points, 1 each, max 4) B4 [4]
- (b) (i) coefficient = $(Z_2 - Z_1)^2 / (Z_2 + Z_1)^2$
= $(6.3 - 1.7)^2 / (6.3 + 1.7)^2$
= 0.33 (unit quoted, then -1) C1
A1 [2]
- (ii) fraction = $\exp(-\mu x)$
= $\exp(-23 \times 4.1 \times 10^{-2})$
= 0.39 C1
A1 [2]
- (iii) intensity = $0.33 \times 0.39^2 \times I$
= $0.050 I$ C1
A1 [2]
(do not allow e.c.f. from (i) and (ii) if these answers are greater than 1)

Q7.

- 10 (a) X-ray taken of slice / plane / section
 repeated at different angles
 images / data is processed
 combined / added to give (2-D) image of slice
 repeated for successive slices
 to build up a 3-D image
 image can be viewed from different angles / rotated
- B1
 B1
 B1
 B1
 B1
 B1
 B1
 max 6 [6]

- (b) (i) 16 A1 [1]

- (ii) evidence of deducting 16 then dividing by 3
 to give
- C1
 A1 [2]

3	2
6	5

Q8.

- 11 *either* quartz *or* piezo-electric crystal
 opposite faces /two sides coated (with silver) to act as electrodes
either molecular structure indicated
or centres of (+) and (–) charge not coincident
 potential difference across crystal causes crystal to change shape
 alternating voltage (in US frequency range) applied across crystal
 causes crystal to oscillate / vibrate
 (crystal cut) so that it vibrates at resonant frequency
 (max 6)
- B1
 B1

 B1
 B1
 B1
 B1
 B1 [6]

Q9.

- 10 (a) product of density (of medium) and speed of sound (in the medium) B1 [1]
- (b) α would be nearly equal to 1 M1
either reflected intensity would be nearly equal to incident intensity
or coefficient for transmitted intensity = $(1 - \alpha)$ M1
 transmitted intensity would be small A1 [3]
- (c) (i) $\alpha = (1.7 - 1.3)^2 / (1.7 + 1.3)^2$ C1
 $= 0.018$ A1 [2]
- (ii) attenuation in fat = $\exp(-48 \times 2x \times 10^{-2})$ C1
 $0.012 = 0.018 \exp(-48 \times 2x \times 10^{-2})$ C1
 $x = 0.42 \text{ cm}$ A1 [3]

Q10.

10	strong / large (uniform) magnetic field		B1	
	nuclei precess / rotate about field direction	(1)		
	radio frequency pulse		B1	
	at Larmor frequency	(1)		
	causes resonance / nuclei absorb energy		B1	
	on relaxation / de-excitation, nuclei emit r.f. pulse		B1	
	pulse detected and processed	(1)		
	non-uniform field superposed on uniform field		B1	
	allows position of resonating nuclei to be determined		B1	
	allows for location of detection to be changed	(1)		
	(six points, 1 each plus any two extra – max 8)			[8]

Q11.

11	(a)	(i)	e.m. radiation produced whenever charged particle is accelerated electrons hitting target have distribution of accelerations	M1 A1	[2]
		(ii)	<i>either</i> wavelength shorter/shortest for greater/greatest acceleration <i>or</i> $\lambda_{\min} = hc/E_{\max}$ <i>or</i> minimum wavelength for maximum energy all electron energy given up in one collision/converted to single photon	B1 B1	[2]
	(b)	(i)	hardness measures the penetration of the beam greater hardness, greater penetration	C1 A1	[2]
		(ii)	controlled by changing the anode voltage higher anode voltage, greater penetration/hardness	C1 A1	[2]
	(c)	(i)	long-wavelength radiation more likely to be absorbed in the body/less likely to penetrate through body	B1	[1]
		(ii)	(aluminium) filter/metal foil placed in the X-ray beam	B1	[1]

Q12.

12	(a)	strong uniform (magnetic) field	M1	
		<i>either</i> aligns nuclei		
		<i>or</i> gives rise to Larmor/resonant frequency <u>in r.f. region</u>	A1	
		non-uniform (magnetic) field	M1	
		<i>either</i> enables nuclei to be located		
		<i>or</i> changes the Larmor/resonant frequency	A1	[4]
	(b)	(i) difference in flux density = $2.0 \times 10^{-2} \times 3.0 \times 10^{-3} = 6.0 \times 10^{-5} \text{ T}$	A1	[1]
		(ii) $\Delta f = 2 \times c \times \Delta B$	C1	
		$= 2 \times 1.34 \times 10^8 \times 6.0 \times 10^{-5}$		
		$= 1.6 \times 10^4 \text{ Hz}$	A1	[2]

Q13.

- 10 (a) e.g. beam is divergent/obeys inverse square law
absorption (in block)
scattering (of beam in block)
reflection (at boundaries)
(any two sensible suggestions, 1 each) B2 [2]
- (b) (i) $I = I_0 \exp(-\mu x)$ C1
 $I_0/I = \exp(0.27 \times 2.4)$ A1 [2]
 $= 1.9$
- (ii) $I_0/I = \exp(0.27 \times 1.3) \times \exp(3.0 \times 1.1)$ C1
 $= 1.42 \times 27.1$ A1 [2]
 $= 38.5$
- (c) either much greater absorption in bone than in soft tissue B1 [1]
or I_0/I much greater for bone than soft tissue

Q14.

- 10 (a) sharpness: how well the edges (of structures) are defined B1
contrast: difference in (degree of) blackening between structures B1 [2]
- (b) e.g. scattering of photos in tissue/no use of a collimator/no use of lead grid
large penumbra on shadow/large area anode/wide beam
large pixel size
(any two sensible suggestions, 1 each) B2 [2]
- (c) (i) $I = I_0 e^{-\mu x}$ C1
ratio $= \exp(-2.85 \times 3.5) / \exp(-0.95 \times 8.0)$ C1
 $= (4.65 \times 10^{-5}) / (5.00 \times 10^{-4})$ A1 [3]
 $= 0.093$
- (ii) either large difference (in intensities) M1
or ratio much less than 1.0 A1 [2]
so good contrast
- (answer given in (c)(ii) must be consistent with ratio given in (c)(i))

Q15.

- 10 (a) product of density and speed of sound / wave M1
(density of medium and) speed of sound / wave in medium A1 [2]
- (b) if $(Z_1 - Z_2)$ is small, mostly transmission M1
if $(Z_1 - Z_2)$ is large, mostly reflection M1
(if 'mostly' not stated allow 1/2 marks for these first two marks)
either reflection / transmission also depends on $(Z_1 + Z_2)$
or intensity reflection coefficient $= (Z_1 - Z_2)^2 / (Z_1 + Z_2)^2$ A1 [3]
- (c) e.g. smaller structures can be distinguished B1
because better resolution at shorter wavelength / higher frequency B1 [2]

Q16.

- 11 (a) changing voltage changes energy / speed of electrons M1
 changing electron energy changes maximum X-ray photon energy A1 [2]
- (b) (i) 1. loss of power / energy / intensity B1 [1]
 2. intensity changes when beam not parallel C1
 decreases when beam is divergent A1 [2]
- (ii) ratio = $(\exp \{-2.9 \times 2.5\}) / (\exp \{-0.95 \times 6.0\})$ C1
 = 0.21 (min. 2 sig. fig.) A1 [2]
 (values of both lengths incorrect by factor of 10^{-2} to give ratio of 0.985 scores 1 mark)

Q17.

- 9 (a) product of density (of medium) and speed of sound (in medium) B1 [1]
- (b) difference in acoustic impedance M1
 determines fraction of incident intensity
 that is reflected/amount of reflection A1 [2]
- (c) pulse of ultrasound (directed into body) B1
 reflected at boundary (between tissues) B1
 (reflected pulse is) detected and processed B1
 time for return of echo gives (information on) depth B1
 amount of reflection gives information on tissue structures B1 [5]

Q18.

- 11 (a) CT image: (thin) slice (through structure) B1
 any further detail e.g. built up from many 'slices' / 3-D image B1
 X-ray image: 'shadow' image (of whole structure) / 2-D image B1 [3]
- (b) X-ray image of slice taken from many different angles (1)
 these images are combined (and processed) (1)
 repeated for many different slices (1)
 to build up a 3-D image (1)
 3-D image can be rotated (1)
 computer required to store and process huge quantity of data (1)
 (any five, 1 each to max 5) B5 [5]

Q19.

- 11 large / 1 T magnetic field applied along body (*allow 'across'*) (1)
- | | |
|--|-----|
| r.f. pulse applied | (1) |
| causes hydrogen nuclei / protons | (1) |
| to resonate | (1) |
| (nuclei) return to equilibrium state / after relaxation time | (1) |
| r.f. (pulse) emitted | (1) |
| pulses detected, processed and displayed | (1) |
| resonant frequency depends on magnetic field strength | (1) |
| calibrated non-uniform field enables nuclei to be located | (1) |
- any six points, one mark each B6 [6]
- [Total: 6]

Q20.

- 10 (a) (i) e.m. radiation / photons is produced whenever a charged particle
is accelerated M1
wavelength depends on magnitude of acceleration A1
electrons have a distribution of accelerations A1
so continuous spectrum A0 [3]
- (ii) *either* when electron loses all its energy in one collision
or when energy of electron produces a single photon B1 [1]
- (b) (i) parallel beam (in matter) B1
 $I = I_0 \exp(-\mu x)$ M1
 I , I_0 , (μ) and x explained A1 [3]
- (ii) *either* low-energy photons absorbed (much) more readily
or low-energy photons (far) less penetrating B1
low-energy photons do not contribute to X-ray image B1
low energy photons could cause tissue damage B1 [3]
- [Total: 10]

Q21.

- 10 (a) (i) density $\times$ speed of wave (in the medium) B1 [1]
- (ii) $\rho = (7.0 \times 10^6) / 4100$
 $= 1700 \text{ kg m}^{-3}$ A1 [1]
- (b) (i) $I = I_T + I_R$ B1 [1]
- (ii) 1. $\alpha = (0.1 \times 10^6)^2 / (3.1 \times 10^6)^2$
 $= 0.001$ C1
A1 [2]
2. $\alpha \approx 1$ A1 [1]
- (c) *either* very little transmission at an air-skin boundary M1
(almost) complete transmission at a gel-skin boundary M1
when wave travels in or out of the body A1 [3]
or no gel, majority reflection (M1)
with gel, little reflection (M1)
when wave travels in or out of the body (A1)

Q22.

- 9 (a) (i) edges can be (clearly) distinguished B1 [1]
- (ii) e.g. size of X-ray source / anode / target / aperture
scattering of X-ray beam
pixel size
(any two, 1 each) B2
further detail e.g. use of lead grid B1 [3]
- (b) X-ray image involves a single exposure B1
CT scan: exposure of a slice from many different angles M1
repeated for different slices A1
CT scan involves a (much) greater exposure B1 [4]

Q23.

- 11 (a) (i) $I / I_0 = \exp(-1.5 \times 2.9)$ C1
 $= 0.013$ A1 [2]
- (ii) $I / I_0 = \exp(-4.6 \times 0.95)$
 $= 0.013$ A1 [1]
- (b) attenuation (coefficients) in muscle and in fat are similar B1
attenuation (coefficients) in bone and muscle / fat are different B1
contrast depends on difference in attenuation B1 [3]

Q24.

- 10 (a) background reading = 19 B1 [1]
- (b) A = 2 A1
 B = 5 A1
 C = 9 A1
 D = 3 A1 [4]
 (Allow 1 mark if only subtracts background reading)
- (c) (i) either 5, 14 or 14, 5 (A+D, B+C or v.v.) B1 [1]
- (ii) Three numbers and 'inside' number is 8 (B+D) B1
 Three numbers and 'outside' numbers are either 2,9 or 9,2 (A,C or v.v.) B1 [2]

Q28.

- 10 (a) pulse (of ultrasound) B1
 produced by quartz / piezo-electric crystal (1)
 reflected from boundaries (between media) B1
 reflected pulse detected B1
 by the ultrasound transmitter (1)
 signal processed and displayed B1
 intensity of reflected pulse gives information about the boundary (1)
 time delay gives information about depth (1)
 (four B marks plus any two from the four, max. 6) B2 [6]
- (b) shorter wavelength B1
 smaller structures resolved / detected (*not more sharpness*) B1 [2]
- (c) (i) $I = I_0 e^{-\mu x}$ C1
 ratio = $\exp(-23 \times 6.4 \times 10^{-2})$ C1
 = 0.23 A1 [3]
- (ii) later signal has passed through greater thickness of medium M1
 so has greater attenuation / greater absorption / smaller intensity A1 [2]

Q29.

- 10 (a) nuclei spin/precess B1
 spin/precess about direction of magnetic field B1
 either frequency of precession depends on magnetic field strength
 or large field means frequency in radio frequency range B1 [3]
- (b) non-uniform field means frequency of precession different in different regions of subject B1
 enables location of precessing nuclei to be determined B1
 enables thickness of slice to be varied / location of slice to be changed B1 [3]

Q30.

- 12 (a) series of X-ray images (for one section/slice)
 taken from different angles
 to give image of the section/slice
 repeated for many slices
 to build up three-dimensional image (of whole object) M1
 M1
 A1
 M1
 A1 [5]
- (b) deduction of background from readings
 division by three C1
 C1
- $P = 5 \quad Q = 9 \quad R = 7 \quad S = 13$
- (four correct 2/2, three correct 1/2) A2 [4]

Q31.

- 11 (a) X-ray: flat/shadow/2D image B1
 regardless of depth of object/depth not indicated B1
- CT scan: built up from (many) images at different angles B1
 image is three-dimensional B1
 image can be rotated/viewed at different angles B1 [5]
- (b) (i) $I = I_0 e^{-\mu x}$ C1
 $0.25 = e^{-0.69x}$
 $x = 2.0 \text{ mm}$ (allow 1 s.f.) A1 [2]
- (ii) for aluminium, $I/I_0 = e^{-0.46 \times 2.4}$
 $= 0.33$ C1
 fraction $= 0.33 \times 0.25$
 $= 0.083$ A1 [2]
- (iii) gain/dB $= 10 \lg(I/I_0)$ C1
 $= 10 \lg(0.083)$
 $= (-) 10.8 \text{ dB}$ (allow 2 s.f.) A1
 with negative sign B1 [3]

Q32.

- 11 (a) X-ray beam contains many wavelengths B1
 aluminium filter absorbs long wavelength X-ray radiation M1
 that would be absorbed by the body (and not contribute to the image) A1 [3]
- (b) CT scan consists of (many) X-ray images of a slice M1
 and there are many slices A1
 X-ray image is a single exposure B1
 (so much) greater exposure with CT scan B1 [4]

Q33.

- 11 (a) product of density and speed
density of medium, speed of wave in medium
(not "speed of light", 0/2)

M1
A1 [2]

(b) (i) $\alpha = (6.4 - 1.7)^2 / (6.4 + 1.7)^2$
 $= 0.34$

C1
A1 [2]

(ii) $I/I_0 = e^{-\mu x}$
 $= \exp(-23 \times 3.4 \times 10^{-2})$
 $= 0.46$

C1
C1
A1 [3]

(iii) $I_R/I = (0.46)^2 \times 0.34$
 $= 0.072$

C1
A1 [2]

1. Nov/2023/Paper_9702/41/No.10

Ultrasound and X-rays are both types of wave that are used in medical diagnosis to form images of internal body structures.

(a) Complete Table 10.1 to state, for each type of wave:

- the method of production of the wave
- whether the wave that is detected and used to form the image is the wave that has been absorbed, reflected or transmitted by the internal body structure.

Table 10.1

	ultrasound	X-rays
method of production		
detected wave (absorbed, reflected or transmitted)		

[4]

(b) (i) For one type of wave passing through tissue, the wave has 72% of its initial intensity after it has passed through 6.2 cm of the tissue.

Calculate the linear attenuation coefficient μ of the tissue for this wave.

$$\mu = \dots\dots\dots \text{ cm}^{-1} \quad [2]$$


(ii) Another wave of the same type as in (b)(i) passes through 9.3 cm of the same tissue.

Calculate the percentage of the initial intensity of the wave that is attenuated by the tissue.

percentage attenuated = ... % [2]

[Total: 8]

Fluorine-18 ($^{18}_9\text{F}$) is a radioactive nuclide that is used as a tracer in positron emission tomography (PET scanning). Fluorine-18 decays to a nuclide of oxygen (O) according to



- (a) (i) State what is meant by a tracer.

.....
 [1]

- (ii) State the symbol of the particle that is represented by X and the values of P , Q and R .

X: P :

Q: R : [2]

- (b) (i) Explain how the radioactive decay of fluorine-18 results in the emission from the body of the gamma-ray photons that are detected during a PET scan.

.....

 [2]

- (ii) Explain how the detection of the gamma-ray photons is used to produce an image of the tissue being examined.

.....

 [2]

- (c) The half-life of fluorine-18 is T .
A patient is injected with amount of substance n of fluorine-18.

- (i) Determine an expression for the initial value R_0 of the rate R of production of gamma-ray photons by the tracer, in terms of n , T and the Avogadro constant N_A .

$$R_0 = \dots\dots\dots [3]$$

- (ii) On Fig. 9.1, sketch the variation with time t of R .

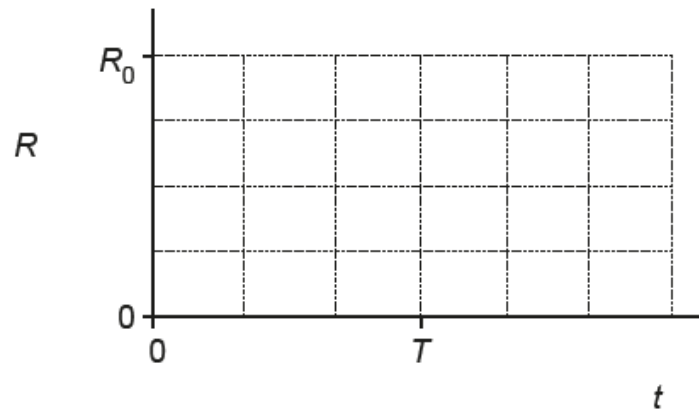


Fig. 9.1

[2]

[Total: 12]

- (a) Table 8.1 shows some data relating to the properties of air, gel and body tissue. The data are given to three significant figures.

Table 8.1

material	density / kg m^{-3}	speed of sound / ms^{-1}	specific acoustic impedance / $\text{kg m}^{-2} \text{s}^{-1}$
air		340	440
gel	1200	1400	
tissue	1090		1.68×10^6

- (i) Show that the specific acoustic impedance of gel is $1.68 \times 10^6 \text{ kg m}^{-2} \text{s}^{-1}$.

[1]

- (ii) Complete Table 8.1 by calculating the missing values to three significant figures. Use the space below for any working that you need.

[2]

- (b) Use the information in (a) to calculate the intensity reflection coefficient for:

- (i) an air–tissue boundary

intensity reflection coefficient = ... [2]

(ii) a gel–tissue boundary.

intensity reflection coefficient = ... [1]

(c) Use your answers in (b) to explain why gel is applied to the skin during ultrasound scanning.

.....

.....

..... [2]

[Total: 8]

- (a) X-rays for use in medical diagnosis are produced in an X-ray tube. In the X-ray tube, charged particles are accelerated towards a metal target by an applied potential difference (p.d.).

(i) State the name of the charged particles that are accelerated by the applied p.d.

..... [1]

(ii) Explain how X-rays are produced at the metal target.

.....

 [2]

(iii) Calculate the minimum wavelength of X-rays produced when the applied p.d. is 5.80 kV.

wavelength = ... m [3]

(b) X-rays pass through a medium that has an attenuation coefficient of 1.4 cm^{-1} .

Calculate the percentage of the X-ray energy that is **absorbed** by a 2.8 cm thickness of this medium.

percentage absorbed = ... % [3]

[Total: 9]

Ultrasound is used to produce diagnostic information about internal body structures.

(a) Explain how ultrasound waves are detected.

.....

.....

.....

..... [3]

(b) An alternating voltage V varies with time t according to

$$V = V_o \sin \omega t.$$

The voltage is applied to an ultrasound probe.

The root-mean-square (r.m.s.) voltage is 66 V. The frequency of the ultrasound generated by the probe is 4.3 MHz.

Determine the values of

(i) V_o

$$V_o = \dots\dots\dots \text{ V [1]}$$

(ii) ω .

$$\omega = \dots\dots\dots \text{ rad s}^{-1} [1]$$

(c) Table 9.1 contains information about air and soft tissue.

Table 9.1

	density / kg m^{-3}	speed of ultrasound / m s^{-1}	specific acoustic impedance /
air	1.30	330	4.3×10^2
soft tissue		1600	1.7×10^6

(i) Determine the unit for the specific acoustic impedance values shown in Table 9.1. [1]

(ii) Calculate the density of soft tissue.

density = ... kg m^{-3} [1]

(iii) Use data from Table 9.1 to explain why ultrasound cannot be used to produce an image inside an air-filled cavity such as the lungs.

.....

.....

.....

..... [2]

[Total: 9]